# P047 Flush Diaphragm Pressure Transmitter



# | Features |

- 316L flush diaphragm structure adopted for pressure connection
- Anti-fouling
- Wide pressure range, can measure absolute pressure, gauge pressure
- Good seal, long-term stable work
- Optional output signal, can be customized

# |Introduction|

P047 adopts flush diaphragm to directly receive pressure signal, takes diffused silicon pressure sensor as sensitive element and uses standard silicone or olive oil as pressure transfer medium. With compact structure, corrosion resistance, vibration resistance and wide range temperature compensation, stainless steel 316L and specially welded flush isolation diaphragm are used for measurement end.

It prevents fouling due to its exposed diaphragm, which is especially applicable to measure viscous fluid pressure with sanitary requirements of health care and food industry, solving problems of fouling, block, cleaning and sanitation. It is also widely applicable to sanitary industries and occasions with fouling forming medium.

# | Applications |

Medicine and health care / Food / Liquor-making / Dairy and drinks / Environmental protection chemical coating / Polyurethane equipment / Paint detection system etc.

H2309-P047

www.eyc-tech.com

Pressure-P047




# |Specification|

Relative pressure : -1 60 bar;Absolute pressure : 0 60 bar
Relative pressure / Absolute pressure
4 20 mA (DC 12 30 V) / 0 10 V (DC 12 24 V)
0.5%F.S.
0.1%F.S.
1.5%F.S. (at -20°C 85°C)
≤1 ms (up to 90%F.S.)
$\geq$ 10×10 <sup>6</sup> pressure cycles
-20°C 85°C
-40°C 85°C
-40°C 85°C
IP65
SS316
DIN 43650


# | Pressure Range |

Pressure range	Overpressure	Burst pressure
$\leq$ 0.7 bar	300%F.S.	500%F.S.
≦ 25 bar	200%F.S.	300%F.S.
≦ 60 bar	150%F.S.	300%F.S.


# | Dimension | Unit:mm

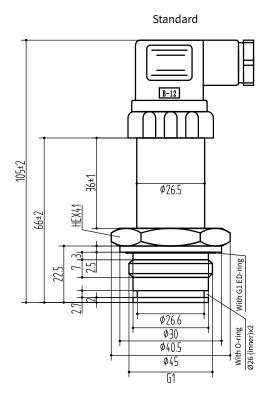

## | Diagram |




#### Voltage output





Pressure-P047 www.eyc-tech.com

### Ordering Guide

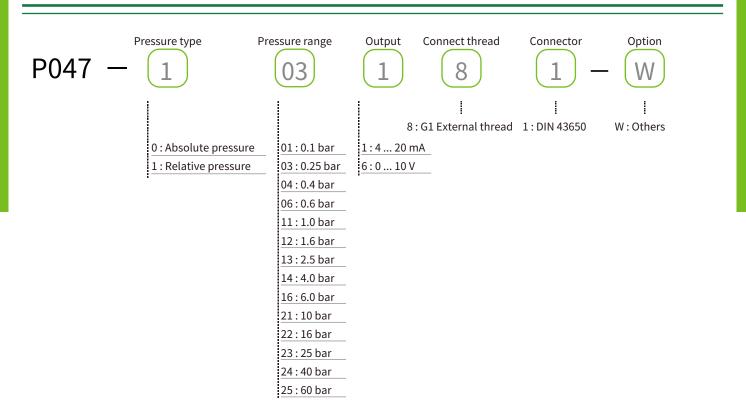

# Additional Option Test Report | For more detailed information please contact us.

#### ILAC / TAF

YUDEN-TECH CO.,LTD. Calibration Laboratory - (ILAC / TAF ) Test report. (TAF accreditation : 3032, complying with ISO / IEC 17025 ) TAF has mutual recognition arrangement with ILAC MRA

Project	Measurand level or range
Pressure transmitter	Gauge pressure : 10 7000 kPa
	Absolute pressure : 20170 kPa

#### ISO 9001

Project	Measurand level or range
Pressure	Relative pressure : $\leq$ 6000 kPa
	Absolute pressure : $\leq$ 1000 kPa
	Differential pressure : 0 500 Pa / 0 1000 Pa / 0 10000 Pa